

Medical Illumination International, Inc. Limited Warranty

This document comprises the general terms of your product's Limited Warranty. This Limited Warranty is applicable to products sold by Medical Illumination International, Inc. or one of its subsidiaries or divisions (collectively, "MI") through one of MI's authorized dealers, distributors or sales representatives (an "Authorized Dealer"). This Limited Warranty is not applicable to any MI product not purchased from an Authorized Dealer. This Limited Warranty extends only to the first retail purchaser of a product and is not transferable or assignable.

Your product is warranted against defective material and/or workmanship, excluding normal replacement parts, for a period of three (3) years from the date of shipment. Normal replacement parts include, but are not limited to, bulbs, sterilizable handles, filters and glass items. This Limited Warranty applies exclusively to the repair or replacement of parts recognized as defective by MI that are in normal use and have not been modified or repaired by unauthorized personnel.

This Limited Warranty is in lieu of all other warranties, expressed or implied, including any implied warranty of fitness for a particular purpose and all other obligations or liabilities, including liability for incidental, special or consequential damages or labor.

In the event of a defect or failure covered under this Limited Warranty, please contact MI immediately by phone (818/838-3025), fax (818/838-3725), email (info@medillum.com) or through our website (<http://www.medillum.com>). Be prepared to give the model number, serial number and full description of the issue. This Limited Warranty will not apply if the MI serial number affixed to the product has been removed, obliterated or defaced.

Our Customer Service department will attempt to solve the problem over the phone. If it becomes necessary, we will determine, in our sole discretion, the best way to address the issue. We may require that the product be sent to our factory for repair. In limited instances, we may dispatch an authorized service technician. No product serviced by other than our authorized service technician will be covered by this Limited Warranty.

In the event we determine that your product needs to be repaired, either onsite or by return to our factory, please do not continue to use your product. MI is not responsible for any costs, expenses, losses or damage resulting from your continued use of the product prior to its authorized repair. MI is not responsible for costs or expenses incurred for loss of use of the product.

If we require the return of the product to our factory, you will be provided with a Return Authorization number. Products sent to the factory without a Return Authorization number will not be accepted. It is your obligation to arrange for return shipment of your product to the factory for warranty service, which shall be at your expense. Your Product must be returned to our factory within thirty (30) days of the date of the Return Authorization. Carefully package the product and return it, freight prepaid and insured, with the Return Authorization number clearly marked on the outside of the box, to Medical Illumination International, Inc., 19749 Dearborn Street, Chatsworth, CA 91311, RA# _____.

Damage resulting from inadequate packing is not covered by this warranty, and shipping insurance does not cover damage due to inadequate packing. MI cannot be held responsible for in-transit loss or damage. In the event that freight-related damage should occur, we will notify you immediately so that you can file a damage claim with the freight carrier.

Within the warranty period, MI will evaluate your returned product, repair as appropriate, and ship the product back to you with freight costs prepaid by MI. In the event that damage or failure is discovered that is not covered by this Limited Warranty, we will contact you for your approval of all costs that may be incurred prior to commencing any repairs.

This Limited Warranty does not cover the following:

- Any field labor or outside services, including, but not limited to, electricians, contractors, installation services, routine maintenance or other repair services.
- Damage to the product resulting from tampering, accident, abuse, negligence, alteration or other causes unrelated to problems with material and/or workmanship.
- Damage due to improper installation, use, cleaning or maintenance, as outlined in the Installation and Service Manual.
- Labor costs associated with removing, re-packaging for shipment or reinstalling product

Limited Warranty, Rev 8-23



USER GUIDE FOR MI-300 EXAM LIGHT



Medical Illumination International
19749 Dearborn Street
Chatsworth, CA 91311
(818) 838-3025

Intended Use: General Lighting Applications

Specifications:

Light Intensity 30,000 LUX at 24"
LED Type/Life CoB / 50,000 hours
Operating Voltage: 100VAC-240VAC/50-60Hz
Light Head Input Voltage 24VDC
Warranty..... 3 years (limited)


Component Checklist:

MI-300 Light Head / Flexible Neck.....1
Upright.....1
Floor Base.....1
Casters.....5
Power Supply Module1

Unpack the components and assemble as follows:


Attach the Castors to the Floor Base:

Insert the Casters into the Base. The Casters should rotate freely and the Base should roll around easily.




Attach the Upright to the Floor Base:

Lower and longer threaded side of the Upright into the Base and securely tighten.



Attach the Flexible Neck to the Upright:

Position the Light Head/Flexible Neck onto the top of the upright and thread onto the upright until tight.

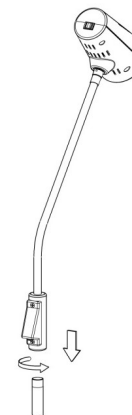

Attach the power:

Plug the Power Cord into the receptacle on the Flexible Neck/Power Input Module and then plug the Power Supply into the wall receptacle. Use the rocker switch at the back of the unit to turn on/off and select intensity

Operating. Positioning and Cleaning the Light:

- The switch at the rear of the light provides for HIGH-OFF-LOW function.



- To position the Light Head, securely hold the Flexible Neck with one hand and position the Light Head to the desired position with the other hand.
- Use mild soap and water to clean the exterior of the light. Never use harsh detergents or chemicals.