

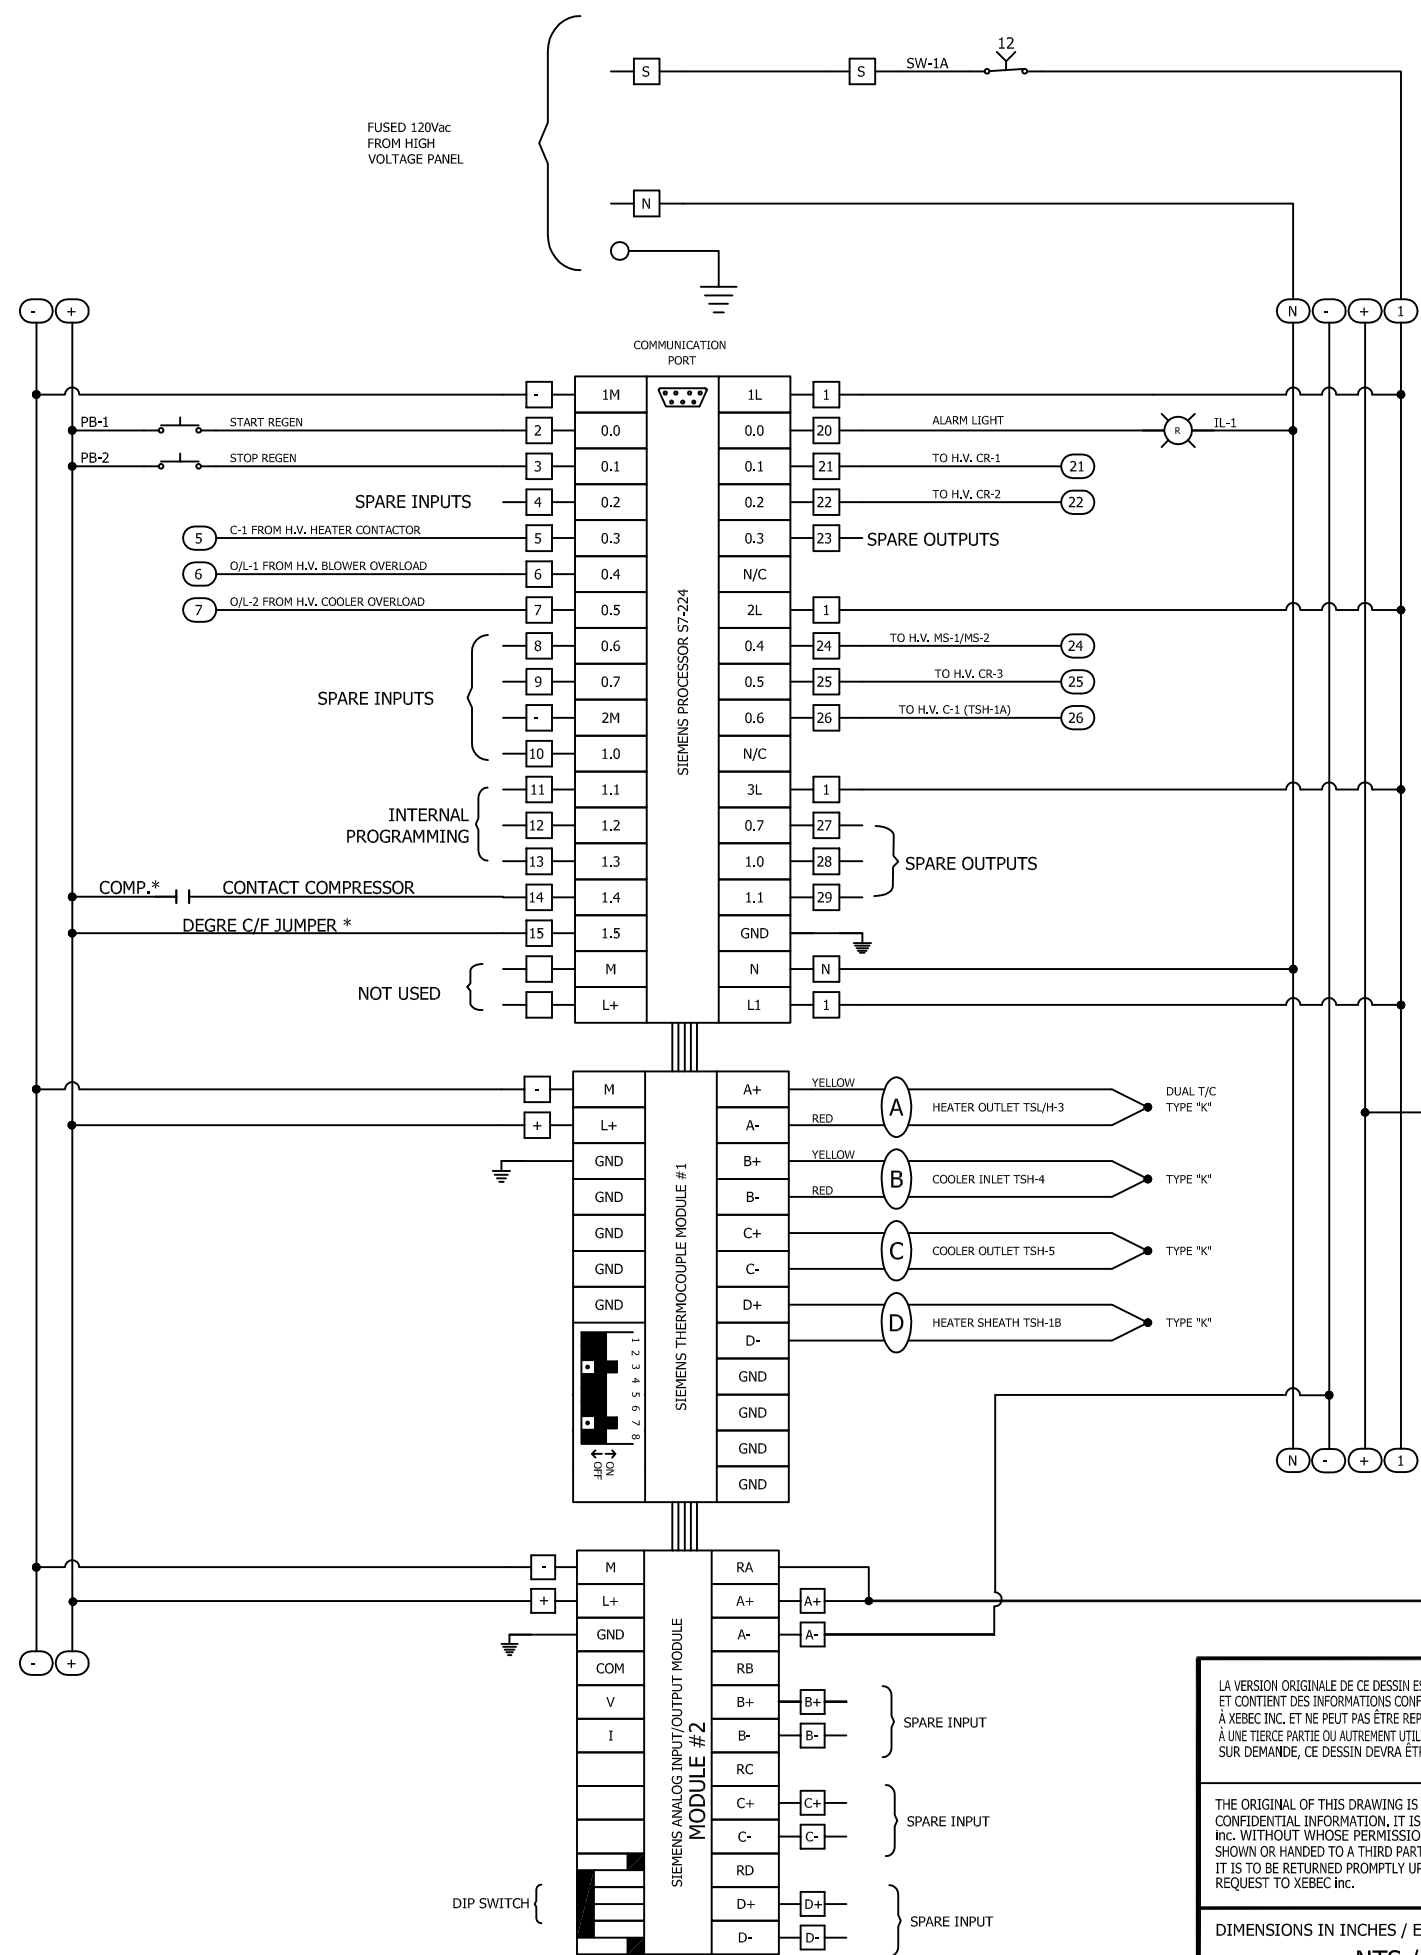


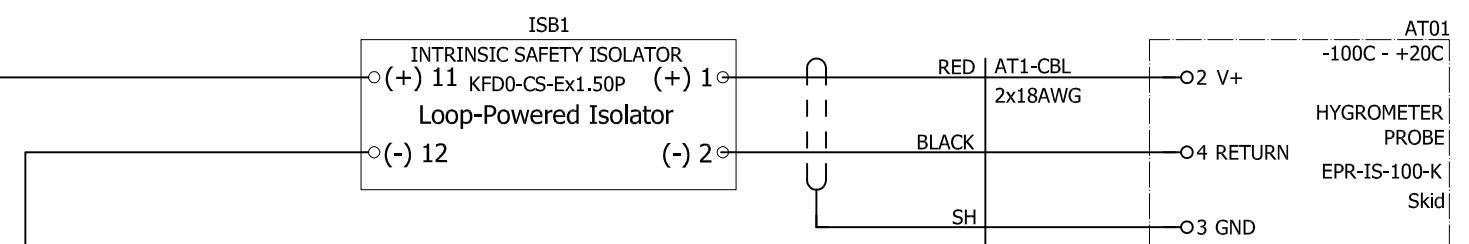

***NOTES:**
JUMPER IN °F STANDARD
JUMPER OUT °C

*COMPRESSOR CONTACT RECOMMENDED
TO BE INSTALLED
(SEE MANUAL FOR DETAIL)

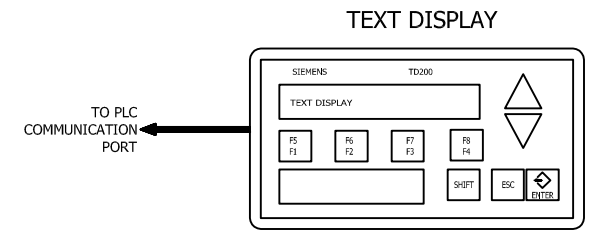

4-20mA SIGNAL CHARACTERISTICS
4mA = -148F/-100C
20mA= +68F/+20C

THE WIRE / CABLE CONNECTED BETWEEN "R+" AND "R-"MUST NOT EXCEED
500 OHMS RESISTANCE AND MAKE SURE TO FOLLOW THE CERTIFICATION FOR
CABLE SELECTION AND CIRCUIT LENGTH, THIS MUST INCLUDE ALL
MONITORING INSTRUMENTS BEING USED ON THIS LOOP.

LA VERSION ORIGINALE DE CE DESSIN EST PROTÉGÉE PAR COPYRIGHT ET CONTIENT DES INFORMATIONS CONFIDENTIELLES. IL APPARTIENT À XEBEC INC. ET NE PEUT PAS ÊTRE REPRODUIT, MONTRÉ OU DONNÉ À UNE TIERCE PARTIE OU AUTREMENT UTILISÉ, SANS SON CONSENTEMENT. SUR DEMANDE, CE DESSIN DEVRA ÊTRE RETOURNÉ À XEBEC INC.						 730 Boul. INDUSTRIEL, BLAINVILLE (QUÉBEC), J7C 3V4 CANADA TEL.: (450) 979-8700 1-877-469-3232 SANS FRAIS FAX.: (450) 979-7869	
THE ORIGINAL OF THIS DRAWING IS COPYRIGHT AND CONTAINS CONFIDENTIAL INFORMATION. IT IS THE PROPERTY OF XEBEC inc. WITHOUT WHOSE PERMISSION IT MAY NOT BE COPIED, SHOWN OR HANDED TO A THIRD PARTY OR OTHERWISE USED AND IT IS TO BE RETURNED PROMPTLY UPON REQUEST TO XEBEC inc.							
	00	NEW DRAWING/NOUVEAU DESSIN FROM E207035			06/07/11		PD
	REV.	DESCRIPTION			DATE		NAME NOM
DIMENSIONS IN INCHES / EN POUCES SCALE/ECHELLE : NTS / NON		DRAWN / DESSINÉ	CHECKED / VÉRIFIÉ	APPROVED / APPROUVÉ	TITLE / TITRE STRNGX TD-200 CONTROL PANEL	DWG NO / NUMÉRO DE DESSIN E1210105	PAGE 1 OF/DE 1
	NAME / NOM	DB	PD	PD			
	DATE	06/07/11	06/07/11	06/07/11			